


# Color Difference Report

Specimen Information		
	Standard	Sample
Name	Prin***U	PCnoir®5317
Material		
Condition	Φ4mm, SCE, UV Cut None	Φ4mm, SCE, UV Cut None
Date Time	4/7/2026 1:40:03 PM	4/7/2026 1:46:48 PM

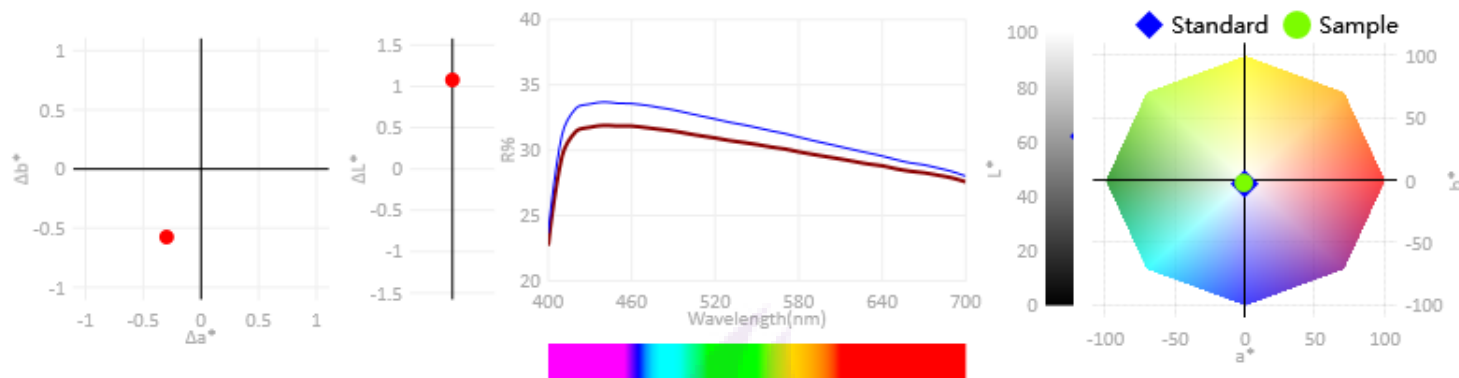

### Tolerance

	ΔE*ab
D65/10°	1.000
A/2°	1.000
F2/2°	1.000

### Color Indexes

		L*	a*	b*	Sum of K/S	MY Carbon
D65/10°	Standard	61.97	-1.19	-1.83	--	51.75
	Sample	63.05	-1.49	-2.40	93.08	49.96
A/2°	Standard	61.67	-1.65	-2.37	--	52.27
	Sample	62.66	-2.12	-3.07	93.08	50.62
F2/2°	Standard	61.78	-0.69	-2.25	--	52.08
	Sample	62.80	-0.86	-2.93	93.08	50.38

### Color Diff.

	ΔL*	Δa*	Δb*	ΔE*ab	Judgement
D65/10°	1.08	-0.30	-0.58	1.26	Fail
A/2°	0.99	-0.47	-0.70	1.30	Fail
F2/2°	1.02	-0.18	-0.68	1.24	Fail

Test: Alfred      Audit: Karry  
 Instrument Model: X-rite Ci64