


Color Difference Report

Specimen Information		
	Standard	Sample
Name	Prin***U	PCnoir®5319
Material		
Condition	Φ4mm, SCE, UV Cut None	Φ4mm, SCE, UV Cut None
Date Time	4/7/2026 1:40:03 PM	4/7/2026 1:48:13 PM

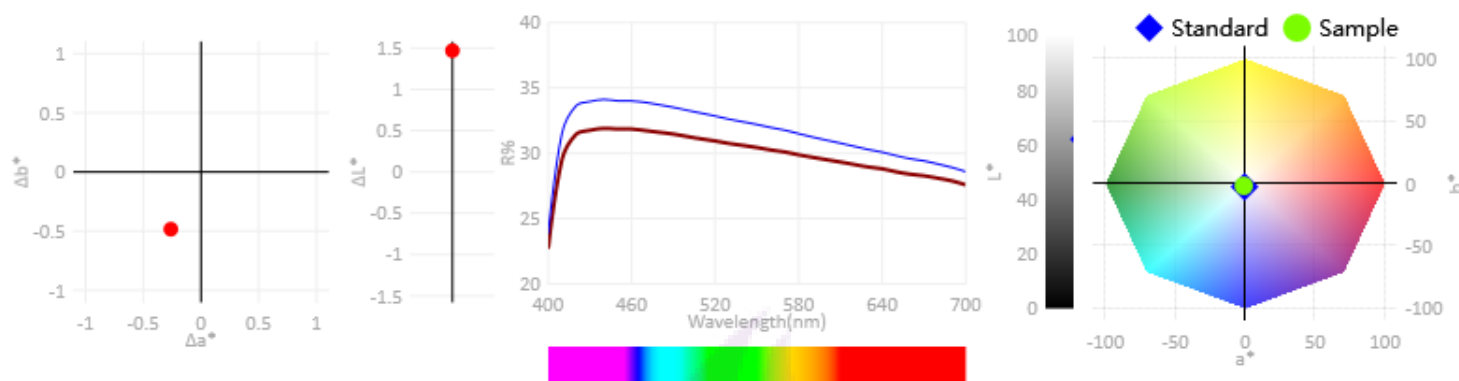

Tolerance

	ΔE*ab
D65/10°	1.000
A/2°	1.000
F2/2°	1.000

Color Indexes

		L*	a*	b*	Sum of K/S	MY Carbon
D65/10°	Standard	61.97	-1.19	-1.83	--	51.75
	Sample	63.44	-1.45	-2.31	90.47	49.32
A/2°	Standard	61.67	-1.65	-2.37	--	52.27
	Sample	63.06	-2.06	-2.96	90.47	49.95
F2/2°	Standard	61.78	-0.69	-2.25	--	52.08
	Sample	63.20	-0.84	-2.83	90.47	49.72

Color Diff.

	ΔL*	Δa*	Δb*	ΔE*ab	Judgement
D65/10°	1.47	-0.26	-0.48	1.57	Fail
A/2°	1.39	-0.41	-0.59	1.57	Fail
F2/2°	1.42	-0.16	-0.58	1.54	Fail

Test: Alfred Audit: Karmy
 Instrument Model: X-rite Ci64