


# Color Difference Report

Specimen Information		
	Standard	Sample
Name	Prin***U	PCnoir®2419
Material		
Condition	Φ4mm, SCE, UV Cut None	Φ4mm, SCE, UV Cut None
Date Time	4/7/2026 1:40:03 PM	4/7/2026 1:44:25 PM

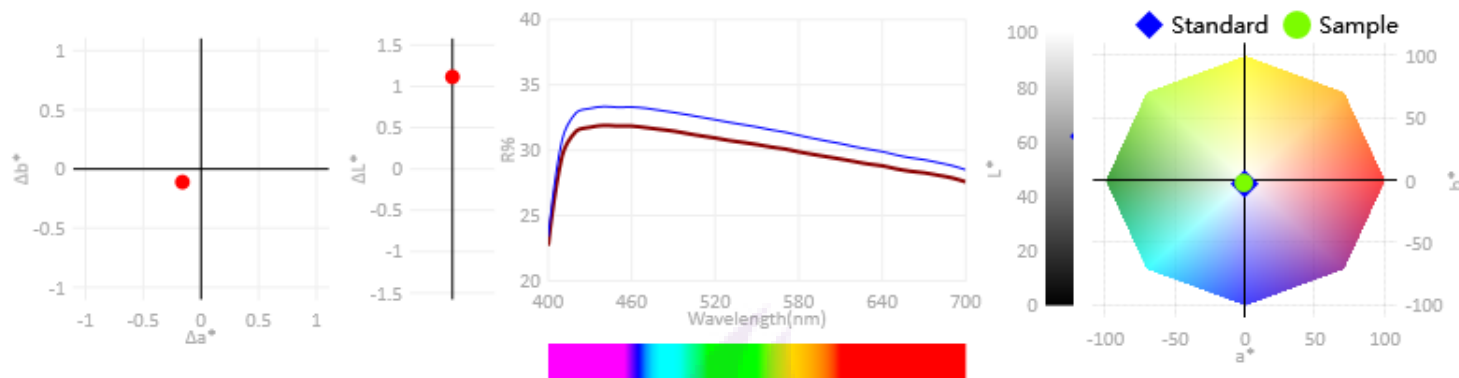

### Tolerance

	ΔE*ab
D65/10°	1.000
A/2°	1.000
F2/2°	1.000

### Color Indexes

		L*	a*	b*	Sum of K/S	MY Carbon
D65/10°	Standard	61.97	-1.19	-1.83	--	51.75
	Sample	63.09	-1.35	-1.94	92.75	49.90
A/2°	Standard	61.67	-1.65	-2.37	--	52.27
	Sample	62.75	-1.85	-2.54	92.75	50.46
F2/2°	Standard	61.78	-0.69	-2.25	--	52.08
	Sample	62.88	-0.79	-2.39	92.75	50.26

### Color Diff.

	ΔL*	Δa*	Δb*	ΔE*ab	Judgement
D65/10°	1.12	-0.16	-0.11	1.13	Fail
A/2°	1.09	-0.20	-0.17	1.12	Fail
F2/2°	1.10	-0.11	-0.14	1.11	Fail

Test: Alfred      Audit: Karry  
 Instrument Model: X-rite Ci64