


Color Difference Report

Specimen Information		
	Standard	Sample
Name	PC®noir 1000	PC®noir 1100
Material		
Condition	Φ4mm, SCE, UV Cut None	Φ4mm, SCE, UV Cut None
Date Time	3/31/2026 10:50:18 AM	3/31/2026 10:52:03 AM

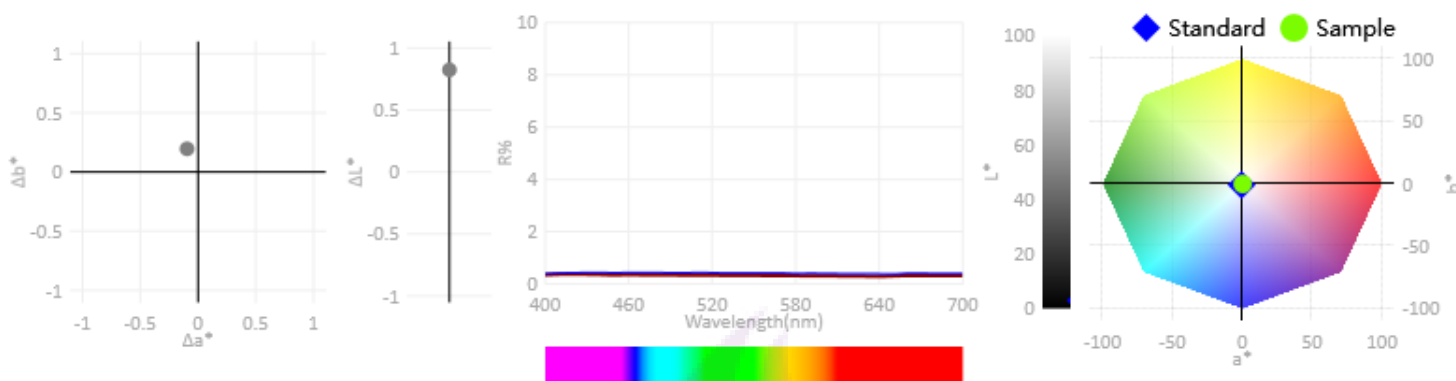

Tolerance

	D65/10°	A/2°	F2/2°
ΔE*ab	1.000	1.000	1.000

Color Indexes

	D65/10°		A/2°		F2/2°	
	Standard	Sample	Standard	Sample	Standard	Sample
L*	2.95	3.77	2.89	3.72	2.91	3.74
a*	-0.15	-0.25	-0.26	-0.31	-0.09	-0.16
b*	-0.48	-0.28	-0.54	-0.38	-0.57	-0.37
C*	0.50	0.37	0.60	0.49	0.58	0.40
h°	252.21	228.61	244.01	230.46	261.00	246.56
MY Carbon	248.61	237.90	249.48	238.53	249.23	238.31
Sum of K/S	--	79.49	--	79.49	--	79.49

Color Diff.

	D65/10°	A/2°	F2/2°
ΔL*	0.82	0.83	0.83
Δa*	-0.09	-0.05	-0.07
Δb*	0.20	0.16	0.20
ΔE*ab	0.85	0.85	0.86
Judgement	Pass	Pass	Pass

Test: Alfred Audit: Karry

Instrument Model: X-rite Ci64