


# Color Difference Report

Specimen Information		
	Standard	Sample
Name	PC®noir B	PC®noir 1000
Material		
Condition	Φ4mm, SCE, UV Cut None	Φ4mm, SCE, UV Cut None
Date Time	3/31/2026 10:50:03 AM	3/31/2026 10:50:18 AM

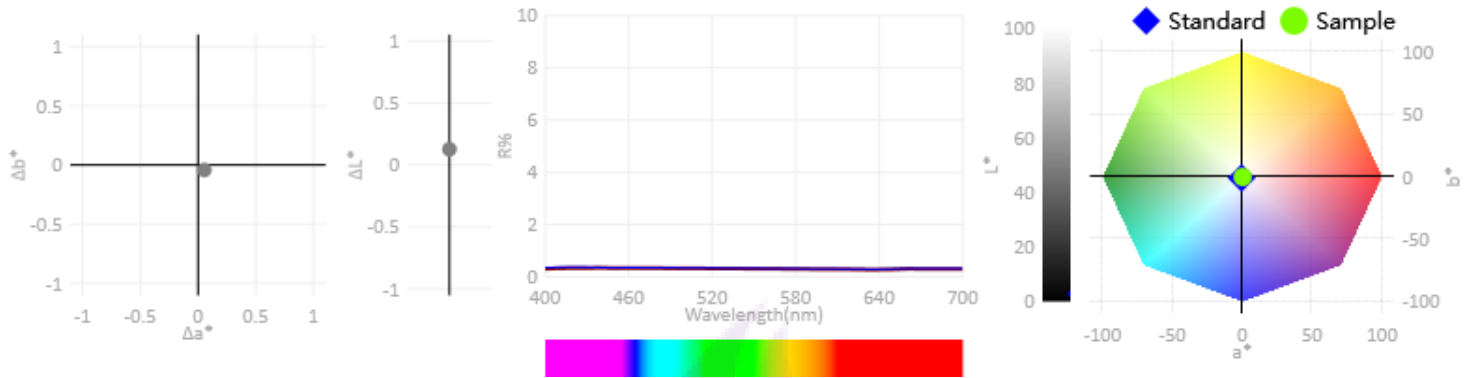

**Tolerance**

	D65/10°	A/2°	F2/2°
ΔE*ab	1.000	1.000	1.000

**Color Indexes**

	D65/10°		A/2°		F2/2°	
	Standard	Sample	Standard	Sample	Standard	Sample
L*	2.82	2.95	2.76	2.89	2.78	2.91
a*	-0.21	-0.15	-0.30	-0.26	-0.13	-0.09
b*	-0.43	-0.48	-0.52	-0.54	-0.53	-0.57
C*	0.48	0.50	0.60	0.60	0.55	0.58
h°	244.51	252.21	240.31	244.01	256.47	261.00
MY Carbon	250.53	248.61	251.48	249.48	251.23	249.23
Sum of K/S	--	94.84	--	94.84	--	94.84

**Color Diff.**

	D65/10°	A/2°	F2/2°
ΔL*	0.13	0.13	0.13
Δa*	0.05	0.04	0.04
Δb*	-0.04	-0.01	-0.03
ΔE*ab	0.14	0.14	0.14
Judgement	Pass	Pass	Pass

Test: Alfred      Audit: Karry  
 Instrument Model: X-rite Ci64